

# Development of a Sensitive LC/MS Assay for Measuring Thyroid Hormones T3 and T4 in Late-Fetal and Neonatal Rat Samples

Elizabeth A. Groeber, Seth R. Bell, Joelle Lucarell, Changyu Quang, Liam Moran, Michael Badamy, and Prāgati Coder

## 1 Introduction

Drugs and chemicals have the potential to perturb thyroid hormone homeostasis with associated deficits in neurological development and function. Guidelines published by the Organization for Economic Co-operation and Development (OECD), as well as the US EPA, require the evaluation of circulating levels of T3, T4, and thyroid stimulating hormone (TSH) in fetal (Gestation Day (GD) 20) and neonatal specimens to address this risk. Sensitive assays capable of measuring T3, T4, and TSH are required and traditional electrochemiluminescent immunoassays (ECLIA) are inadequate. In response, a highly sensitive LC-MS/MS method was developed.

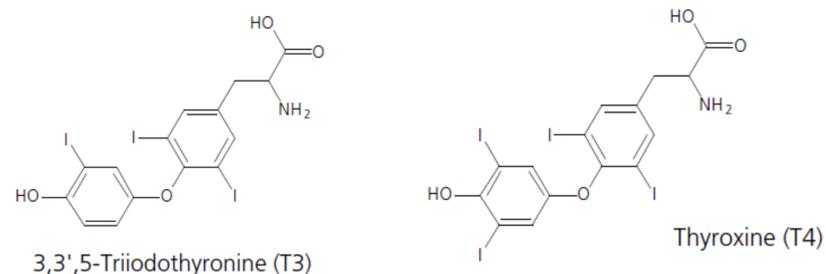


Figure 1. Chemical structure of critical Thyroid Hormones 3,3',5-Triiodothyronine (T3) and Thyroxine (T4).

## 2 Methods

- The analytical method is conducted on wet ice and uses a Supported Liquid Extraction (SLE) in a 96-well plate format.
- A surrogate analyte approach utilizes stable isotopically labeled T3 and T4 in adult rat serum thus having matching calibration, quality control, and sample matrices.
- Only 50 $\mu$ L of rat serum is required for simultaneous T3 and T4 quantitation.
- Validated range allows for multiplexed analysis of developmental and adult samples in the same analytical run.

### Instrument Parameters

#### LC Conditions

##### Parameter:

LC System:	Shimadzu Nexera®
Column:	Agilent ZORBAX RRHD Eclipse Plus 95Å Phenyl-Hexyl, 2.1 x 50 mm, 1.8- $\mu$ m particle size
Mobile Phase A:	0.1% Glacial Acetic Acid in Milli-Q water
Mobile Phase B:	0.1% Glacial Acetic Acid in Acetonitrile
Sample Temperature:	4°C
Column Temperature:	50°C

#### MS Conditions

MS System:	API 5500
Ionization Mode:	ESI Positive Mode
IS Voltage:	5500
Temperature:	650°C

## 3 Results

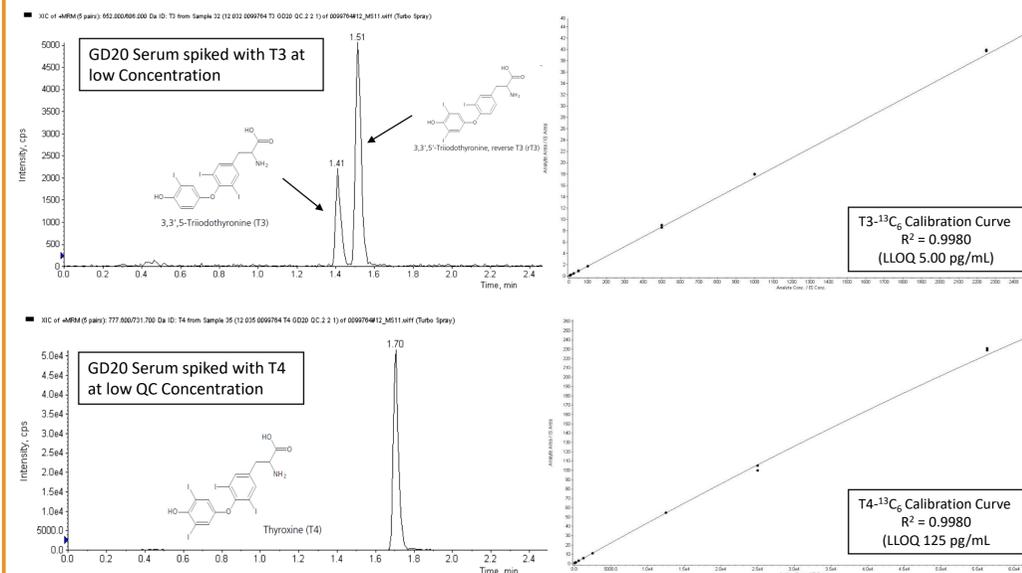


Figure 2. To the left are representative chromatograms of native GD20 rat serum quality control samples overspiked at the low QC concentration with T3 and T4, respectively. These quality control samples demonstrate the ability to quantitate extremely low concentrations of thyroid hormones in sample matrix. To the right are surrogate analyte calibration lines utilizing stable label isotope T3 and T4.

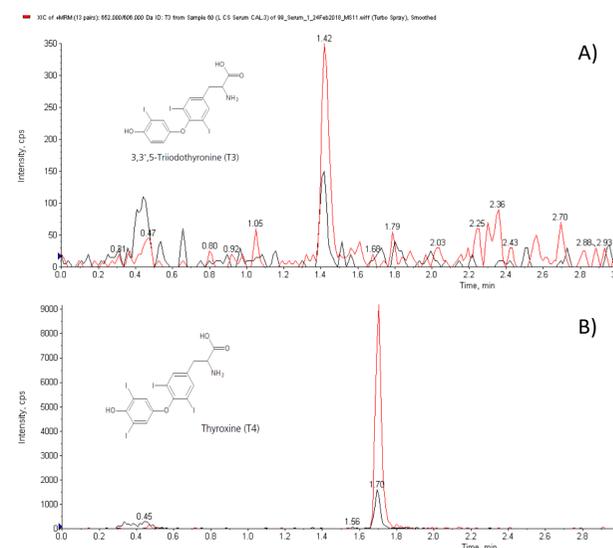


Figure 3. Thyroid hormones are monitored simultaneously for a quantitative ion (Red Trace) and a confirmatory ion (Black Trace). This adds an additional layer of identification points for species identification in agreement with several guidance documents for environmental and organic residue analyses. Shown are the quantitative and monitor ions for A) T3 at 10.0 pg/mL and B) T4 at 250 pg/mL adding confidence to identification even at extremely low sample concentrations.

LC-MS/MS Assay and Performance Summary		
	T3	T4
LLOQ (pg/mL)	5.00	125
Range (pg/mL)	5.00 – 2,500	125 – 62,500
Inter-day % RE (%CV) at LLOQ (n=18) [ <sup>13</sup> C-labeled]	+5.4 (14.6)	+2.4 (11.3)
Inter-day % RE (%CV) overspiked GD20 serum (n=9/12)	+1.1 (12.4)	-10.4 (12.3)
Inter-day % RE (%CV) overspiked adult serum (n=9)	-0.8 (5.9)	+4.2 (6.2)

LC-MS/MS Assay Rat Serum Summary		
	T3 (pg/mL)	T4 (pg/mL)
Gestation Day 20 (Litters pooled, regardless of sex)	12.2 – 20.9	2566 – 6090
Postnatal Day 4 (litters pooled, regardless of sex)	91.3 – 273	17,200 – 35,900
Postnatal Day 13 (mixed gender)	NA	55,500 – 109,000
Adult (Female)	317 – 763	15,500 – 40,600
Adult (Male)	267 – 550	16,200 – 47,100

Figure 4. The method for T3 and T4 was validated according to guidelines for bioanalytical method validation (FDA 2001 and EMA BMV 2011). All testing results demonstrated passing criteria, allowing the method's use in supporting sample analysis.

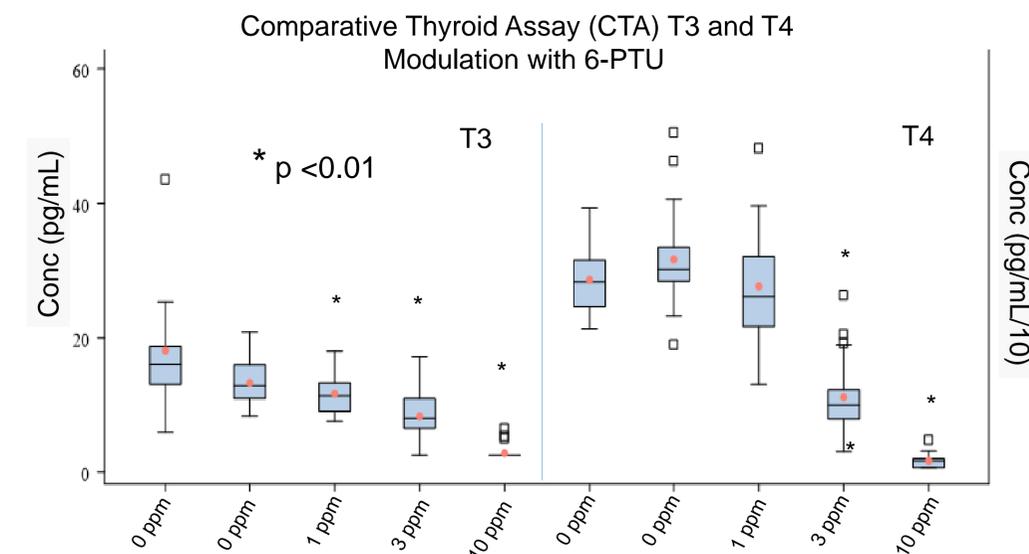


Figure 5. Rat T3 and T4 hormones levels were monitored as part of a Charles River sponsored Comparative Thyroid Assay (CTA) study. Data presented are for Gestational Day 20 rat fetuses. Both T3 and T4 were observed to downwardly modulate in response to 6-n-Propyl-2-thiouracil (PTU) exposure ( $p < 0.01$ ).

## 4 Conclusions

LC-MS/MS offers sensitivity enhancements capable of determining T3 and T4 during the period of thyroid development in rats (late gestation and early neonatal period). The low sample volume (50  $\mu$ L) improves over ELISA methodology (>200  $\mu$ L) to achieve T3 and T4 measurements. The method was successfully applied to determine levels of T3 and T4 in a CTA study including demonstrating modulation in response to 6-PTU exposure. The assay presented improves on prior methodologies by capturing low level T3 and T4 via their enhanced sensitivity and lower LLOQs.